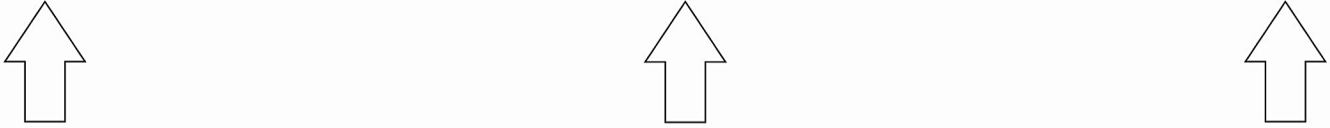

Place this end along edge of overbed table facing the resident

Distance capability of sensor 8-10 ft
Horizontal angle 110-130 degrees Vertical angle 10-20 degrees

Direction of Monitoring Beam

HeadBoard

Pillow

Foot of Bed

Overbed table can be positioned anywhere along dotted line facing towards head of bed

Place Movement Sensor Unit on Here

Switch needs to be pressed hard to switch on/off

Please refer to instructions on reverse side for height of overbed table.

Place the connecting cable from the Room Unit into the Nurse Call socket

IMPORTANT NOTICE

IF A USER FAILS TO POSITION AND SWITCH ON THE SENSOR CORRECTLY IT WILL NOT PICK UP ANY MOVEMENT

Live-Link
6 Milrig Holdings
Kirknewton
EH27 8DE
01506 884404
http://www.nursecallalarms.co.uk